



# **INSTRUCTION MANUAL**

---

**BALDWIN**<sup>TM</sup> - Series

**HEATED FILTER PROBES**

**GENERAL PURPOSE SERIES**

**Model 32C**

---

Perma Pure LLC  
P.O. Box 2105, 8 Executive Drive  
Toms River, NJ 08754  
[www.permapure.com](http://www.permapure.com)

Tel: 732-244-0010  
Tel: 800-337-3762 (toll free US)  
Fax: 732-244-8140  
Email: [info@permasure.com](mailto:info@permasure.com)

# TABLE OF CONTENTS

---

A: Specifications.....	3
B: Limited Warranty.....	4
C: Principle of Operation.....	5
D: Maintenance.....	6
E: Troubleshooting.....	7
F: Spare Parts.....	8
Appendix: .....	9

# A: SPECIFICATIONS

---

## General Specifications

Probe	18" Stinger probe, 0.5" dia x .065" wall, 316L SS tubing
Calibration	Integral calibration on both sides of filter element
Heater Jacket Temp Control	External regulated (standard)
Connections	1/4" male pipe nipple mount; 1/2" male pipe thread adapter
Connectors	1/4" cal gas, 3/8" sample line
Thermocouple	Type K
Heat-shrink Boot	7" length, 2.75" min expanded I.D. nose
O-rings	Viton <sup>®</sup>
Gaskets	Graphoil
Dimensions	14" x 12" x 8" HWD (w/o Stinger probe)
Weight	30 lbs

## Operating Specifications

Calibration Gas Requirement	20 psig, 6-10 LPM
Probe Operating Temperature	375°F (190°C)
Input Voltage	110 standard (220 optional) VAC, 50/60 Hz

## Material Specifications

Enclosure Material	NEMA 4 Steel
Probe Stinger	316L SS tubing (standard) Schedule 40 Schedule 80 Durinert <sup>®</sup> coated Hastelloy <sup>®</sup>
Heater Type	Silicone rubber blanket w/ metal snap closures
Enclosure Insulation Material	1/8" thick silicone, medium density
Filter Chamber Material	316 stainless steel
Filter Element Types	10 micron sintered SS (standard) 5, 20 micron sintered SS 2 micron ceramic 2 micron SS screen mesh

# **B: LIMITED WARRANTY**

---

## **Perma Pure LLC WARRANTY and DISCLAIMERS**

Perma Pure (Seller) warrants that product supplied hereunder shall, at the time of delivery to Buyer, conform to the published specifications of Seller and be free from defects in material and workmanship under normal use and service. Seller's sole obligation and liability under this warranty is limited to the repair or replacement at its factory, at Seller's option, of any such product which proves defective within one year after the date of original shipment from seller's factory (or for a normal usable lifetime if the product is a disposable or expendable item) and is found to be defective in material or workmanship by Seller's inspection.

Buyer agrees that (1) any technical advice, information, suggestions, or recommendations given to Buyer by Seller or any representative of Seller with respect to the product or the suitability or desirability of the product for an particular use or application are based solely on the general knowledge of Seller, are intended for information guidance only, and do not constitute any representation or warranty by Seller that the product shall in fact be suitable or desirable for any particular use or application; (2) Buyer takes sole responsibility for the use and applications to which the product is put and Buyer shall conduct all testing and analysis necessary to validate the use and application to which Buyer puts the product for which Buyer may recommend the use or application of the product by others; and (3) the characteristics, specifications, and/or properties of the product may be affected by the processing, treatment, handling, and/or manufacturing of the product by Buyer or others and Seller takes no responsibility for he nature or consequence of such operations or as to the suitability of the product for the purposes intended to be used by Buyer or others after being subjected to such operations.

SELLER MAKES NO OTHER WARRANTY, EXPRESS OR IMPLIED, OF THE PRODUCT SUPPLIED HEREUNDER, INCLUDING, WITHOUT LIMITATION, IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR PARTICULAR PURPOSE, AND ALL SUCH WARRANTIES ARE HEREBY EXPRESSLY EXCLUDED. SELLER SHALL HAVE NO LIABILITY FOR LOSS OF PROFITS, OR SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES UNDER ANY CIRCUMSTANCES OR LEGAL THEORY, WHETHER BASED ON NEGLIGENCE, BREACH OF WARRANTY, STRICT LIABILITY, TORT, CONTRACT, OR OTHERWISE. SELLER SHALL IN NO EVENT BE LIABLE IN RESPECT OF THIS ORDER AND OR PRODUCT DELIVERED ON ACCOUNT OF THIS ORDER FOR ANY AMOUNT GREATER THAN THAT PAID TO SELLER ON ACCOUNT OF THIS ORDER.

# C: PRINCIPLE OF OPERATION

---

The Perma Pure Baldwin™-Series Model 32C Heated Filter Probe is designed to be mounted on a stack or duct for use in high particulate applications. Its primary function is to provide a heated environment to maintain sample gas temperatures above dewpoint and remove particulate material from the gas sample. Model 32C features a standard 10 micron sintered stainless steel filter element, an externally-regulated heater jacket, an integral calibration gas port on both sides of the filter element, and a NEMA 4 enclosure.




## Mounting

The Model 32C is designed to be mounted directly on a stack or duct with a 1¼" Schedule 40 male pipe nipple. This pipe nipple can be screwed into a standard ASA flange, either flat or raised face. The probe boot can be heat shrunk to the sample line to eliminate cold spots.

## Calibration

To operate calibration gas to the probe, open the user supplied calibration gas control valve, adjust the cylinder pressure to >25 psig, and adjust the calibration gas flow rate to approximately 20% above the highest gas sample flow rate.

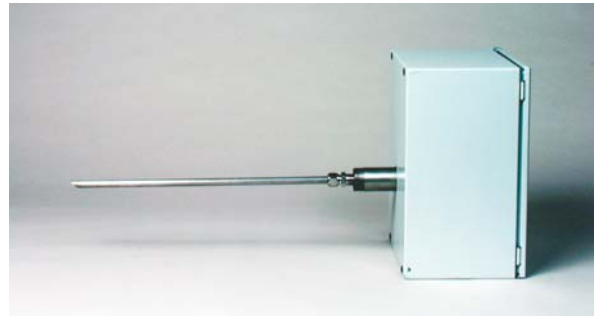

# D: MAINTENANCE

---

The Model 32C does not require routine maintenance for the filter head or externally-regulated probe body heater jacket.

The filter element requires periodic replacement, depending upon application and dust loading. See the attached Spare Parts list for replacement elements.

If the Model 32C is used in conjunction with the Baldwin™-Series Flow Control Drawer, monitoring the sample vacuum will warn the operator when to change the filter element. The operator should log the beginning sample vacuum when the system is first started up.

If the sample vacuum is consistently 25% higher than at start-up, the operator should replace the filter element with a new filter. Visual inspection will also confirm the condition of the filter element.

# E: TROUBLESHOOTING

---

<i>Symptom</i>	<i>Check</i>	<i>Action</i>
115 VAC heater jacket is not heating	Check the resistance between the black and white wires (tied together) and the blue wire. A 200 watt heater @ 115 VAC will draw about 2 amps so the resistance is around 61 ohms.	If the measure is open for heater resistance the fusible link has blown and the jacket should be replaced.
230 VAC heater jacket is not heating	Check the resistance between the black and white power wires using an ohmmeter. A 200 watt heater @ 230 VAC will draw about 1 amp so the resistance is around 245 ohms.	If the measure is open for heater resistance, the fusible link has blown and the jacket should be replaced.
Filter plug cannot be removed from filter housing	Check "O" rings for damage  High particulate loading	Replace "O" rings  Clean the "O" ring sealing surfaces with a clean towel prior to reassembly.

**For further service assistance, contact:**

Perma Pure LLC  
P.O. Box 2105  
8 Executive Drive (08755)  
Toms River, NJ 08754  
Phone: (732) 244-0010  
Fax: (732) 244-8140  
[www.permapure.com](http://www.permapure.com)  
info@permasure.com  
or your local representative

# F: SPARE PARTS

---

## Model 32C (Part Number 4P-32C)

Part No.	Description
1PCG-002	Connector: Heated Line Entry Seal
3FES-015PK	Filter Element Seals: Silicone, Used w/ Screen Mesh 3FES-010 (10 pack)
3FES-010	Filter Element: 316L SS Screen Mesh, 2.0 Micron
3FES-004	Filter Element: 316L SS, 1.25" x 2.975", 10 Micron
3FES-003	Filter Element: 316L SS, 1.25" x 2.975", 20 Micron
3FES-005	Filter Element: 316L SS, 1.25" x 2.975", 5 Micron
3FEC-002	Filter Element: Ceramic 2 Micron
3FEG-001	Filter Element: Glass, 0.1 Micron
3FEG-003	Filter Element: Glass/TFE Coated, 0.7 Micron
4P-FLANGE2	Flange: 2", 150# with Gasket & Bolts
4P-FLANGE3	Flange: 3", 150# with Gasket & Bolts
4P-FLANGE4	Flange: 4", 150# with Gasket & Bolts
4P-FLANGE6	Flange: 6", 150# with Gasket & Bolts
4P-GCS-212	Gas Cooling Spool Piece: w/ 2" Flanges & 12" Spool
4P-GCS-412	Gas Cooling Spool Piece: w/ 4" Flanges & 12" Spool
3PAM-006PK	Gasket: Graphoil 1.25" (10 pack)
3PHH-003	Heater Jacket, Wire-Wound w/ Thermostat & Thermal Fuse ("C" series only)
2HTR-007	Heater Band, 350W
3PAM-028PK	O- Ring: Silicone, 50 Durometer (10 pack)
3PAM-010PK	O- Ring: Viton, 50 Durometer (10 pack)
3PAM-031PK	O-Ring: Pack, Viton, "C" series probes only, 5 ea 1 $\frac{7}{8}$ " OD, 2 $\frac{1}{4}$ " OD
4P-STNG-STD	Stinger, Replacement: 18", 316L SS, $\frac{1}{2}$ " x 0.065"w
2VRS-005	Valve: Check, 10 psig, $\frac{1}{4}$ " Viton "O" Ring
2VS2-007	Valve: Solenoid, 2 Way, 120VAC/60Hz, 100 psig, Hi Temp
2VS2-006	Valve: Solenoid, 2 Way, 220VAC/50Hz, 100 psig, Hi Temp



# APPENDIX:

---

## DIRECT EXTRACTIVE FILTER PROBES

### General Purpose Model 32C

#### Application

The Baldwin<sup>TM</sup>-Series Model 32C Heated Filter Probe is designed to be mounted on a stack or duct for use in low particulate applications. Its primary function is to provide a heated environment to maintain sample gas temperatures above dewpoint and remove particulate material from the gas sample. Model 32C features an external regulated heater jacket, a standard 10 micron sintered stainless steel filter element, an integral calibration gas port on both sides of the filter element, and a NEMA 4 enclosure.



#### General Specifications

Probe	
Calibration	Integral calibration on both sides of filter element
Heater Jacket Temp Control	External regulated (standard)
Connections	1¼" male pipe nipple mount; ½" male pipe thread adapter
Tube Connectors	3/8" sample line, 1/4" calibration gas
Thermocouple	Type K
Heat-shrink Boot	7" length, 2.75" min expanded I.D. nose
O-rings	Viton®
Gaskets	Graphoil®
Dimensions	14 x 12 x 8 in. HWD (w/o Stinger probe) 36 x 30 x 20 cm HWD
Weight	30 lbs 14 kg

#### Operating Specifications

Calibration Gas Requirement	20 psig, 6-10 LPM
Probe Operating Temperature	375°F (190°C)
Input Voltage	110 standard (220 optional) VAC, 50/60 Hz

#### Material Specifications




Enclosure Material	NEMA 4 Steel (standard); NEMA 4X Stainless Steel (optional)
Heater Type	Silicone rubber blanket with metal snap closures
Enclosure Insulation Material	½" thick silicone, medium density
Filter Chamber Material	316 stainless steel
Filter Element Types	10 micron sintered SS (standard) 5, 20 micron sintered SS 2 micron ceramic 2 micron SS screen mesh

Baldwin<sup>TM</sup> is a Trademark of Perma Pure LLC  
 Viton® is a Registered Trademark of DuPont  
 Graphoil® is a Registered Trademark of Union Carbide Corporation



1 2 3 4 5 6 7 8

REV#	DATE	DESCRIPTION	DRAWN	APPROVED
0	00/00/00	INITIAL DRAWING	JO	JO
A	03/01/04	CREATED TO TRUE SCALE. NEW TTB	RAW	RAW

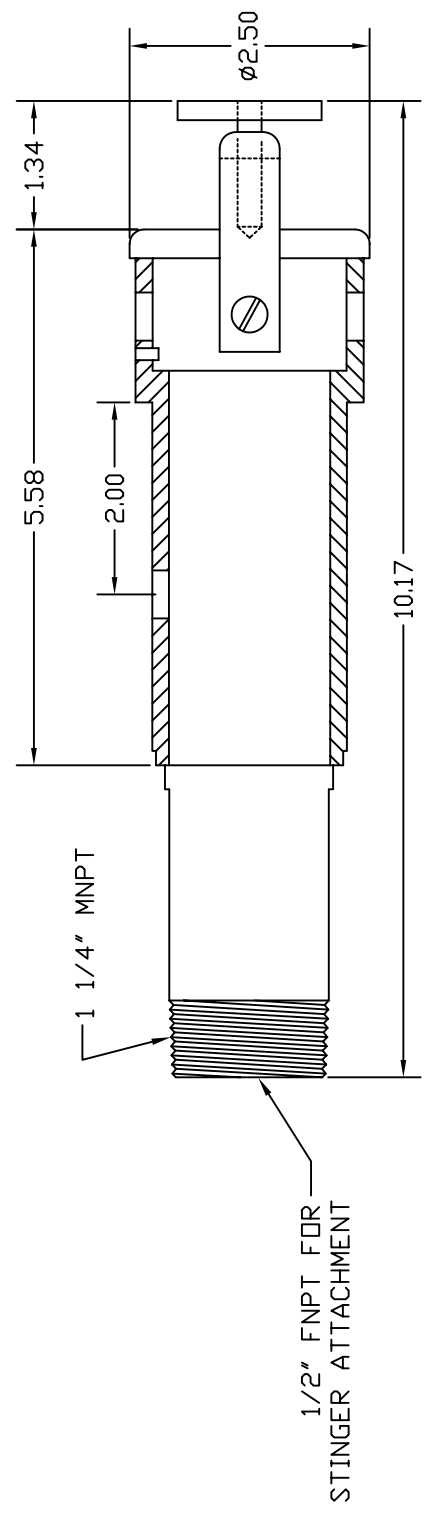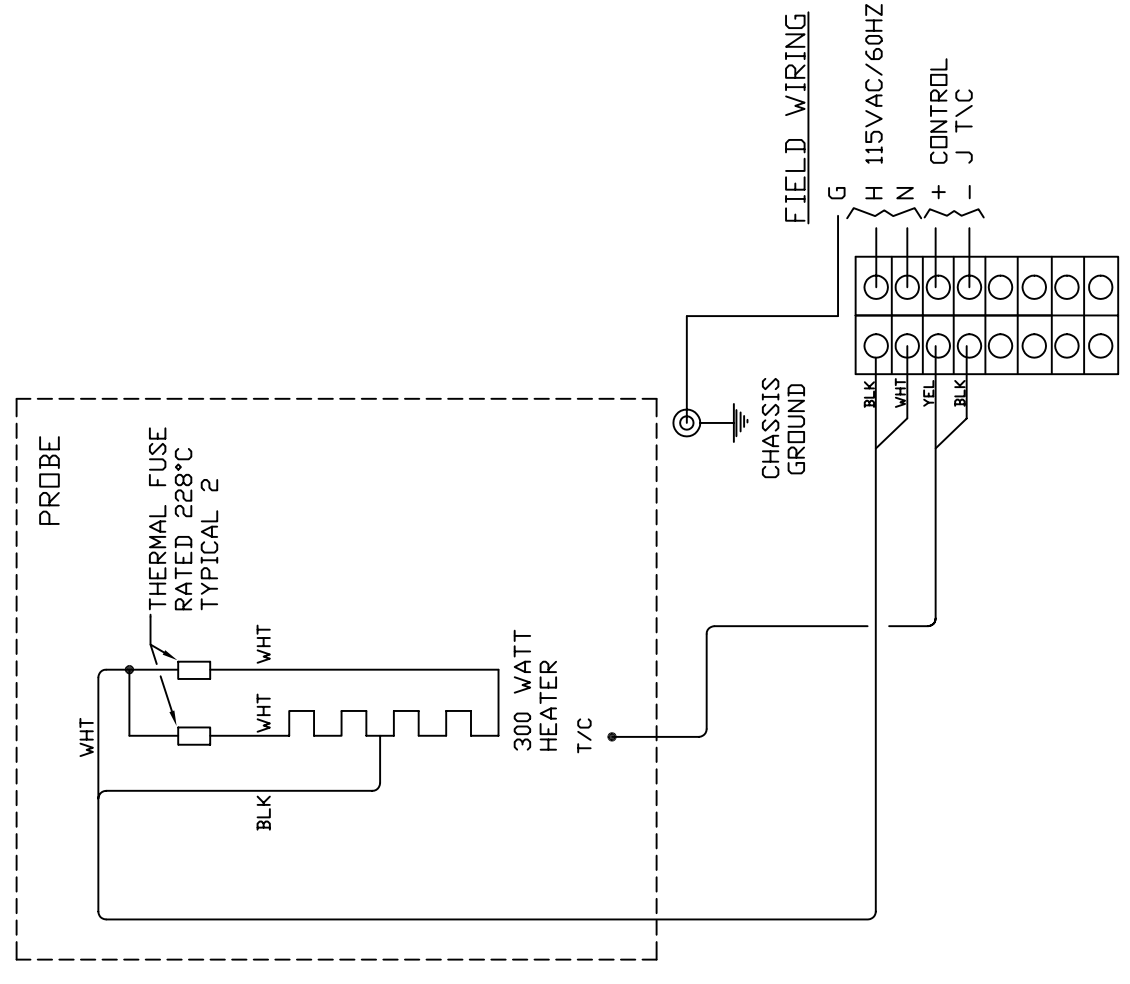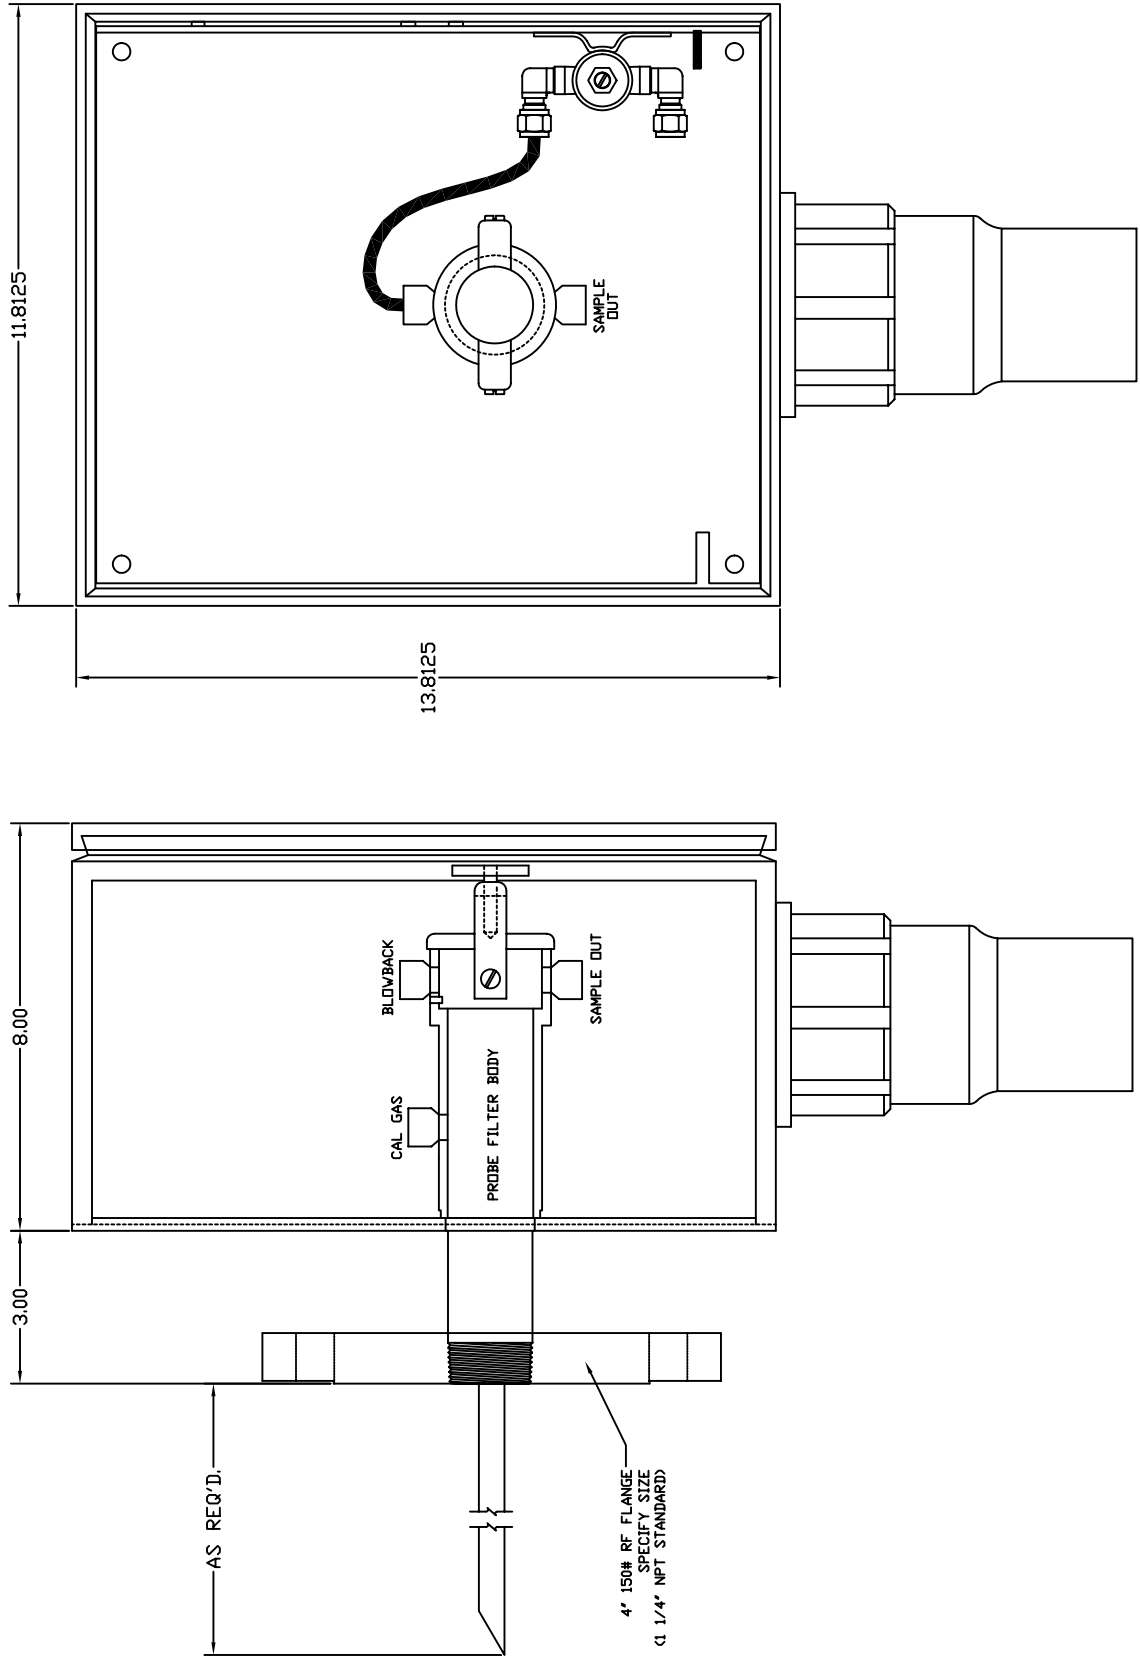

**FILTER PROBE**  
(SCALE = 1/2')

UNLESS OTHERWISE SPECIFIED		TOLERANCE DECIMALS		ANGLES = ±5°		Holes = ±.002-.001	
1	PLACE = ±.02	2	PLACE = ±.02				
3	PLACE = ±.010						
PROPRIETARY INFORMATION THIS DOCUMENT CONTAINS INFORMATION PROPRIETARY TO <b>BALDWIN, INC.</b>		AND IS TO BE USED SOLELY FOR THE PURPOSE FOR WHICH IT IS FURNISHED. THIS DOCUMENT SHALL NOT BE USED FOR ANY OTHER DESIGN, REPAIR, REWORK, OR MANUFACTURING, IN WHOLE OR IN PART. <b>BALDWIN, INC.</b>		DATE 05/12/02		DATE	
BALDWIN, INC. www.baldwinUSA.com				BALDWIN, INC.			
ITEM QTY		DESCRIPTION		MANUF.			
USED FOR		DESCRIPTION					
MODEL NUMBER		DESCRIPTION					
DRAWN BY JO		DATE 05/12/02		PART DESCRIPTION <b>BALDWIN, INC.</b>			
APP'D				MODEL 32C SAMPLE PROBE ARRANGEMENT DRAWING			
MATERIAL				SIZE SCALE B NTS MODEL 32C			
FINISH				DRAWING/PART NO.			
DESIGN DIMENSIONS ARE IN INCHES ( ) DENOTES MILLIMETER EQUIVALENTS WHEN USED				CAD DIR: S:\SBA\DWG\HEATED FILTER PROBES			
				SHEET 1 OF 1			

D

C

B

A

1 2 3 4 5 6 7 8